


## Artificial intelligence identifies and quantifies colonoscopy blind spots

Some mucosal surfaces on folds and within haustra may not be visualized at all during colonoscopy, and thus precancerous lesions are missed. We describe here preliminary results of an artificial intelligence (AI) technology that identifies and quantifies these “blind spots,” with the aim, potentially, that endoscopists may be directed to them in real time. Anonymized colonoscopy videos were acquired from a single endoscopist with a high (47%) adenoma detection rate (ADR), using Olympus CF and PCF devices (Olympus USA, Valley Forge, Pennsylvania, USA) and high definition recording


(Epiphan, Palo Alto, California, USA). The main AI modalities applied were a recurrent neural network (an AI type particularly suitable for sequential data), that had been trained to compute depth [1, 2] combined with visual simultaneous localization and mapping (SLAM) [3]. The AI software was applied to 76 colonoscopy video sequences from 18 patients, showing colon segments of 4–25 cm in length. This created three-dimensional (3D) reconstructions of the colon segments and then identified blind spots, showing as holes or gaps in the reconstructions, and quantified these non-

visualized areas. The study endoscopist reviewed the reconstructions and validated that the blind spots had not been seen in the colonoscopy video. The last 12 3D reconstructions were done in real time with the video sequence; these were 2–6 seconds in duration, corresponding to colon lengths of 7–25 cm (median 10 cm).


► **Video 1** shows a colonoscopy video alongside the real-time reconstruction highlighting a blind spot. ► **Fig. 1** is an example of a reconstructed segment of colon with no blind spot, while ► **Fig. 2** shows a sequence of video images where

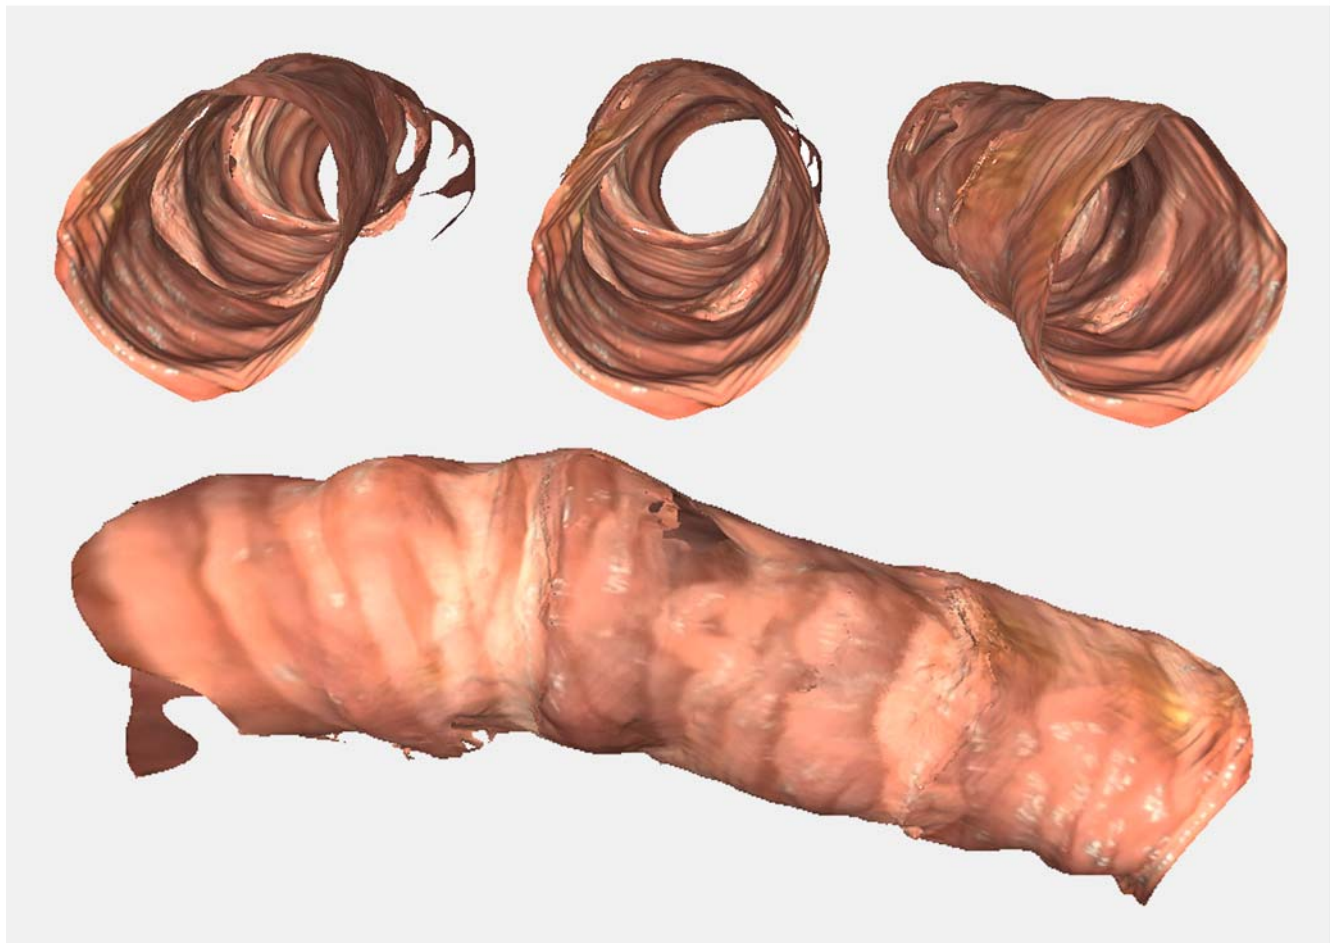

► **Fig. 1** AI-reconstructed segment of the colon with no blind spot.

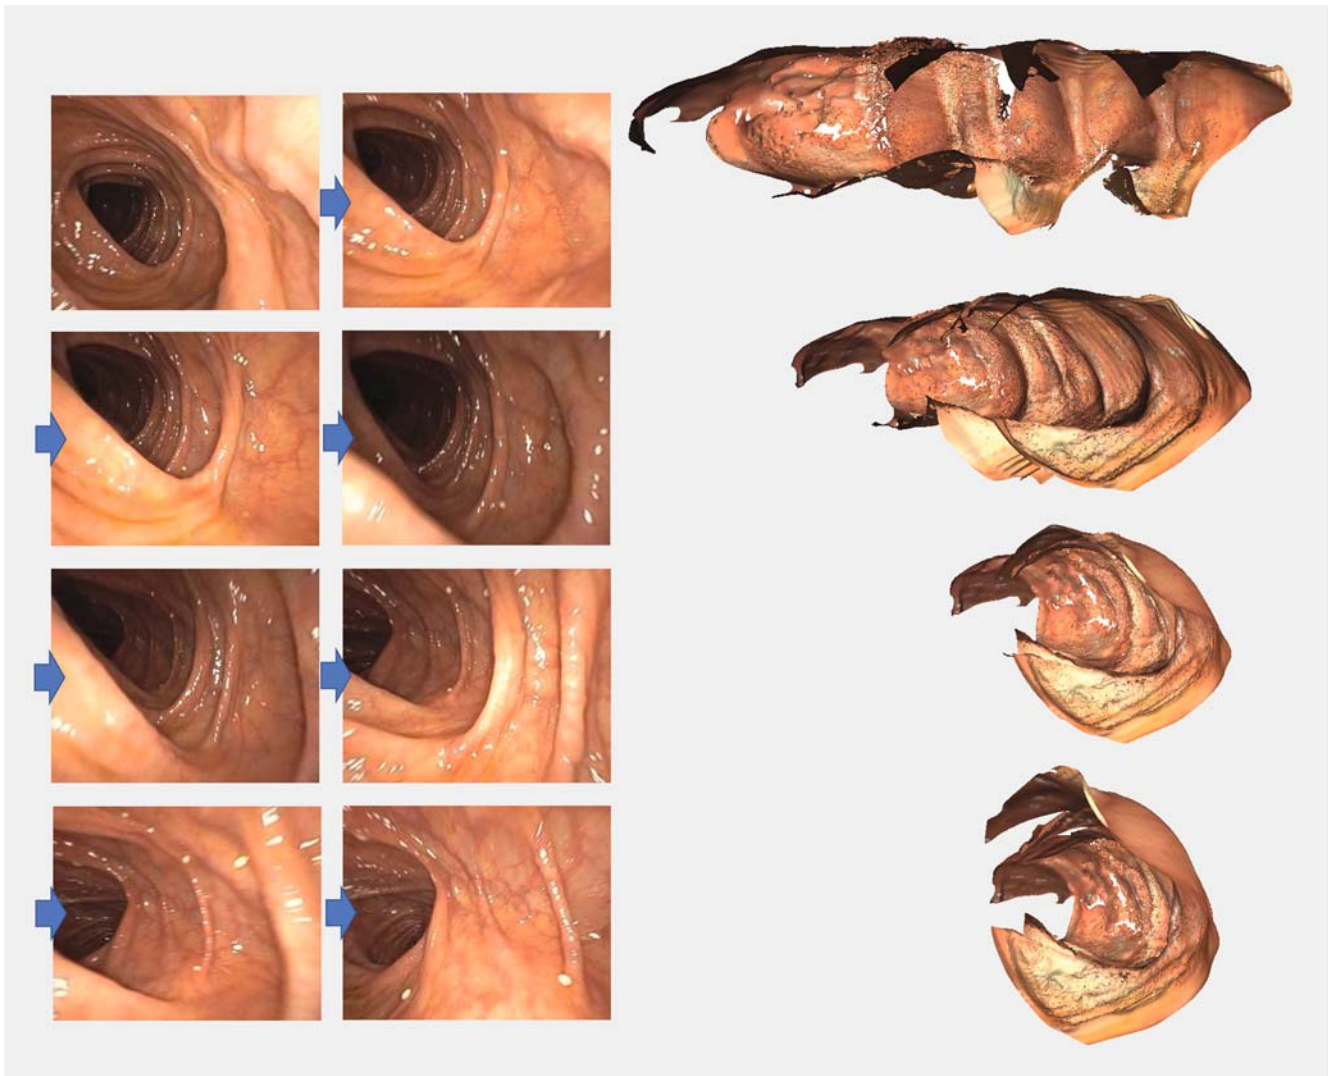

► **Fig. 2** The blind spot of left colon wall missed at colonoscopy is seen as a gap in this reconstruction.

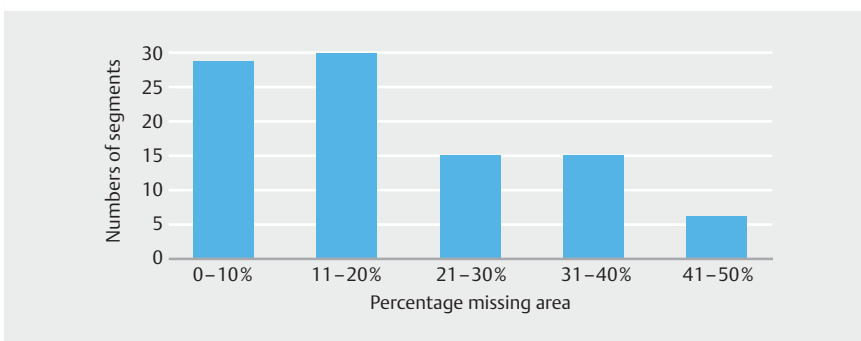

► **Fig. 3** Histogram of frequency of percentage missing area among 76 segments of colonoscopy video.

27%), with a median 19% of surface area being missed despite the high ADR of the operator. ► **Fig. 3** shows the distribution of the differing missed area percentages among the 76 reconstructed colonic segments.


Endoscopy\_UCTN\_Code\_TTT\_1AQ\_2AB

### Funding

National Cancer Institute  
 1-R01-CA158925-01A1  
 Lineberger Comprehensive Cancer  
 Center, University of North Carolina  
 UNC Lineberger Grant for Clinical/  
 Translational research

the left wall of the colon was not visualized because of the camera angle, and the reconstructions with corresponding gaps.

Our system calculated that among the 76 reconstructed segments, the blind spots ranged from 1% to 50% of the total surface area (interquartile range 8.7%–

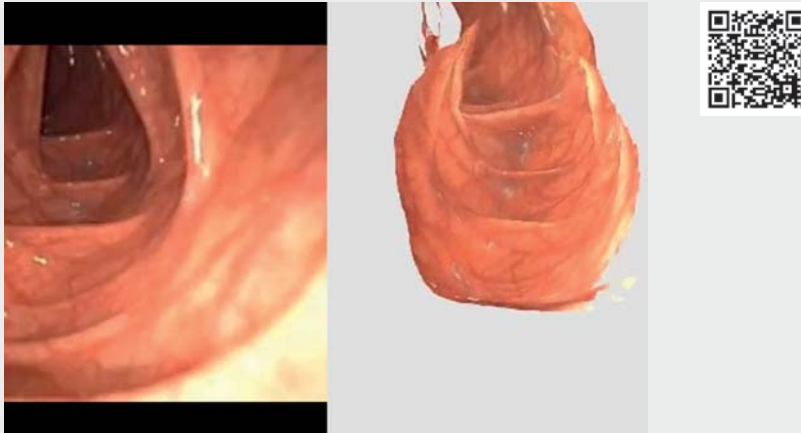

**▶ Video 1** Artificial-intelligence identification and quantification of colonoscopy blind spots. The video shows the colonoscopy video (left) and real-time reconstruction (center and right) which highlights the blind spot in the colon wall.

- [2] Ma R, Wang R, Pizer S, Rosenman J, McGill SK, Frahm J. Real-time 3D reconstruction of colonoscopic surfaces for determining missing regions. Shen D et al. Medical image computing and computer assisted intervention – MICCAI 2019. Lecture Notes in Computer Science, vol 11768. Cham: Springer; 2019
- [3] Engel J, Koltun V, Cremers D. Direct sparse odometry. IEEE Trans Pattern Anal Mach Intell 2018; 40: 611–625

## Bibliography

Endoscopy 2021; 53: 1284–1286

DOI 10.1055/a-1346-7455

ISSN 0013-726X

published online 4.2.2021

© 2021. Thieme. All rights reserved.

Georg Thieme Verlag KG, Rüdigerstraße 14, 70469 Stuttgart, Germany

## ENDOSCOPY E-VIDEOS

<https://eref.thieme.de/e-videos>



*Endoscopy E-Videos* is a free access online section, reporting on interesting cases and new

techniques in gastroenterological endoscopy. All papers include a high quality video and all contributions are freely accessible online.

This section has its own submission website at

<https://mc.manuscriptcentral.com/e-videos>

## Competing interests

All authors are patent holders. Sarah K. McGill and Julian Rosenman have received research funding from Olympus.

## The authors

Sarah K. McGill<sup>1</sup>, Julian Rosenman<sup>2,3</sup>, Rui Wang<sup>3</sup>, Ruibin Ma<sup>3</sup>, Jan-Michael Frahm<sup>2</sup>, Stephen Pizer<sup>3</sup>

- 1 Department of Internal Medicine, Division of Gastroenterology and Hepatology, The University of North Carolina at Chapel Hill, Chapel Hill, North Carolina, USA
- 2 Department of Radiation Oncology, The University of North Carolina at Chapel Hill, Chapel Hill, North Carolina, USA
- 3 Department of Computer Science, The University of North Carolina at Chapel Hill, Chapel Hill, North Carolina, USA

## Corresponding author

**Sarah K. McGill, MD, MSc**

Division of Gastroenterology and Hepatology, University of North Carolina at Chapel Hill School of Medicine, 130 Mason Farm Rd Office Campus Box 7080, Chapel Hill, North Carolina 27599, USA  
Fax: +1-919-966-8929  
mcgills@med.unc.edu

## References

- [1] Wang R, Pizer SM, Frahm J-M. Recurrent neural network for (un-)supervised learning of monocular video visual odometry and depth. Proceedings of the IEEE Conference on Computer Vision and Pattern Recognition. 2019: 5555–5564. Available at: [https://openaccess.thecvf.com/content\\_CVPR\\_2019/html/Wang\\_Recurrent\\_Neural\\_Network\\_for\\_Un-Supervised\\_Learning\\_of\\_Monocular\\_Video\\_Visual\\_CVPR\\_2019\\_paper.html](https://openaccess.thecvf.com/content_CVPR_2019/html/Wang_Recurrent_Neural_Network_for_Un-Supervised_Learning_of_Monocular_Video_Visual_CVPR_2019_paper.html)