

3D MRI of the Knee

Faysal Altahawi, MD¹ Jason Pierce, DO² Mercan Aslan¹ Xiaojuan Li, PhD^{1,3} Carl S. Winalski, MD^{1,3}
Naveen Subhas, MD, MPH¹

¹Section of Musculoskeletal Imaging, Imaging Institute, Cleveland Clinic, Cleveland, Ohio

²Diagnostic Radiology Residency, Imaging Institute, Cleveland Clinic, Cleveland, Ohio

³Department of Biomedical Engineering, Lerner Research Institute, Cleveland Clinic, Cleveland, Ohio

Address for correspondence Naveen Subhas, MD, MPH, Section of Musculoskeletal Imaging, Imaging Institute, Cleveland Clinic, Diagnostic Radiology A21, 9500 Euclid Avenue, Cleveland, OH 44195 (e-mail: subhasn@ccf.org).

Semin Musculoskelet Radiol 2021;25:455–467.

Abstract

Three-dimensional (3D) magnetic resonance imaging (MRI) of the knee is widely used in musculoskeletal (MSK) imaging. Currently, 3D sequences are most commonly used for morphological imaging. Isotropic 3D MRI provides higher out-of-plane resolution than standard two-dimensional (2D) MRI, leading to reduced partial volume averaging artifacts and allowing for multiplanar reconstructions in any plane with any thickness from a single high-resolution isotropic acquisition. Specifically, isotropic 3D fast spin-echo imaging, with options for tissue weighting similar to those used in multiplanar 2D FSE imaging, is of particular interest to MSK radiologists. New applications for 3D spatially encoded sequences are also increasingly available for clinical use. These applications offer advantages over standard 2D techniques for metal artifact reduction, quantitative cartilage imaging, nerve imaging, and bone shape analysis. Emerging fast imaging techniques can be used to overcome the long acquisition times that have limited the adoption of 3D imaging in clinical protocols.

Keywords

- ▶ 3D knee MRI
- ▶ isotropic resolution
- ▶ multiplanar reconstruction
- ▶ cartilage imaging

Although two-dimensional (2D) multiplanar fast spin-echo (FSE) acquisitions have been the cornerstone of knee magnetic resonance imaging (MRI) for many decades, three-dimensional (3D) MRI has been increasingly incorporated into clinical protocols as the technology has evolved.^{1–10} Knee MRI has often been at the forefront of evolving musculoskeletal (MSK) MRI research and trends. The development of new 3D sequences that provide benefits over 2D acquisitions for various applications, such as cartilage, bone, and hardware imaging, in addition to new acceleration techniques that allow images to be acquired more quickly, has made 3D imaging more applicable for routine knee MRI evaluation.^{11,12}

Although most clinical protocols still use multiplanar 2D FSE imaging for primary knee joint assessment, many practices add a single 3D isotropic or near-isotropic acquisition, often reconstructed into multiple planes with multiplanar reconstructions (MPRs). First used with a focus on evaluating

articular cartilage to detect small chondral lesions prone to partial volume averaging on 2D imaging, newer 3D FSE sequences are now increasingly being performed to assess other structures, such as menisci, ligaments, tendons, and nerves.^{2,13–15} Three-dimensional sequences are especially beneficial for these evaluations because nonorthogonal MPRs can be performed along or perpendicular to the course of these structures.^{3,15,16}

Aside from providing value in reducing partial volume averaging and offering the ability to perform MPRs, various 3D sequences afford additional benefits for specific applications. Three-dimensional spatially encoded MRI has a central role in many metal artifact reduction sequences used throughout the MSK system, including the knee.¹¹ Compositional and quantitative MRI techniques increasingly use 3D MRI and are typically developed for imaging of knee cartilage, usually in the research setting.^{9,17–20} However, as acceleration and automation technologies continue to

evolve, these advanced imaging techniques should become more practical in a clinical workflow.^{12,17,21–27}

In this review, we discuss 3D MRI sequences currently available for the knee, as well as the advantages and limitations of 3D MRI relative to routine 2D knee MRI. We also describe emerging techniques for 3D MRI, including acceleration and automated quantification techniques.

Current Techniques

Three-dimensional spatially encoded MRI is performed by excitation of the entire imaged volume rather than the slice-by-slice method used for 2D imaging. The typical frequency and phase encoding are used for the in-plane resolution (voxel dimension along the x-axis and y-axis) of the image. However, phase encoding is also used in the slice direction (voxel dimension along the z-axis) and determines slice thickness. Three-dimensional isotropic spatial resolution refers to the acquired resolution of the volume and indicates that slice thickness is at or near in-plane resolution with no or little gap between slices, allowing MPRs to be created in any desired imaging plane without substantial loss of image resolution.

Many 3D MRI sequences have been created and investigated for MSK evaluation of the knee (► **Table 1**).^{3,9,28,29} The availability of these various 3D sequences depends on the scanner strength and vendor. Many of the sequences first developed for 3D knee MRI were gradient-recalled echo (GRE) techniques because more commonly used spin-echo and FSE techniques could not be performed in a reasonable length of time before the introduction of newer technologies.^{30–32} Although useful for evaluating articular cartilage, GRE sequences have contrast properties that are not well suited for evaluating other structures, such as menisci, tendons, ligaments, and bones.

Table 1 Summary of imaging applications of 3D imaging and types of 3D sequences used for each application

Imaging application	3D sequences
Morphological cartilage assessment	3D FSE, bright fluid 3D GRE, dark fluid 3D GRE
Meniscus assessment	3D FSE
Nerve assessment	3D FSE, DW-PSIF, diffusion tensor imaging
Whole joint assessment	3D FSE
Metal artifact reduction ^a	SEMAC, MAVRIC
Segmentation	3D FSE, bright fluid 3D GRE, dark fluid 3D GRE
Compositional cartilage assessment ^{a,b}	T1 ρ , T2, T2*, dGEMRIC, DWI, sodium 23

Abbreviations: 2D, two-dimensional; 3D, three-dimensional; dGEMRIC, delayed gadolinium-enhanced MRI of cartilage; DW-PSIF, diffusion-weighted reversed fast imaging with steady-state precession; FSE, fast spin-echo; GRE, gradient-recalled echo; MAVRIC, multi-acquisition variable-resonance image combination; SEMAC, slice encoding for metal artifact correction.

^aThese sequences are typically nonisotropic 3D spatially encoded sequences.

^bCompositional sequences typically have both 3D and 2D spatially encoded acquisition options.

GRE sequences are still commonly used in clinical practice, however, because they are commercially available on most scanners including scanners with lower magnetic field strengths. Advances in scanner and coil technology have since allowed for the development of 3D FSE sequences that can achieve signal characteristics similar to 2D FSE proton-density (PD) or T2 weighting, increasing the clinical utility of 3D acquisitions.^{33,34} Although these sequences allow for complete joint evaluation, their availability is limited on older scanners, and they work best on 3-T scanners.⁹

3D Gradient-recalled Echo for Morphological Assessment

Although early 3D GRE sequences had lower nonisotropic resolutions, high-resolution isotropic or near-isotropic voxels amenable to MPRs have been available for many years.^{3,28,30} Although various 3D GRE acquisitions with different types of contrast weighting are available from different vendors, the sequences can be broadly classified into two categories: dark fluid signal sequences and bright fluid signal sequences. Because GRE sequences do not have a refocusing pulse, they are predisposed to susceptibility artifacts that can limit evaluation after surgery and reduce conspicuity of bone marrow edema signal. Additionally, the typically short echo times make these sequences subject to magic angle artifact that limits the evaluation of low-signal curving structures such as menisci, ligaments, and tendons. As a result, research on bright and dark fluid GRE sequences in knee MRI has focused mainly on cartilage evaluation because there is typically good contrast between fluid, articular cartilage, and bone.

Both bright and dark fluid 3D GRE sequences can be advantageous for the morphological assessment of knee cartilage.^{3,32} Many early studies found that dark fluid GRE sequences such as the 3D spoiled GRE sequence could be used to measure articular cartilage volume and thickness with good accuracy.⁸ These high-resolution isotropic dark fluid GRE morphological sequences have often been considered the standard for cartilage morphology assessment in the research setting, but they can have long scan times and a compromise of resolution or quality when optimized for clinically feasible acquisition times (► **Fig. 1**). Bright fluid high-resolution 3D GRE sequences, such as the 3D double-echo steady-state sequence, offer faster acquisition times and favorable fluid-to-cartilage contrast, resulting in improved assessment of the cartilage surface (► **Fig. 2**).^{8,29} Many clinical practices, including our own, therefore use 3D GRE acquisitions, more often bright fluid techniques, in addition to multiplanar 2D FSE sequences, to assess articular cartilage on MRI scanners that do not have clinically feasible 3D FSE sequences available (typically older systems and those with lower field strengths).

3D Fast Spin Echo for Morphological Assessment

Most vendors now offer 3D FSE sequences that use techniques such as parallel imaging, variable flip angles, long echo trains, and partial k-space filling to achieve clinically feasible imaging times.^{33,34} Because 3D FSE acquisitions rely on acceleration techniques that decrease image signal-to-noise ratio (SNR) to reduce acquisition times, these techniques perform better on 3-T systems because they produce images

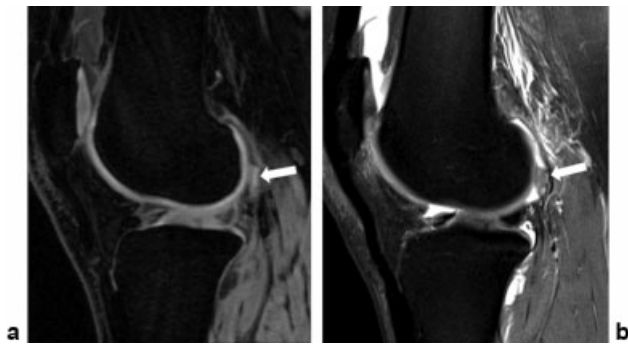


Fig. 1 (a) Displaced intra-articular cartilage fragment (arrow) from a lateral femoral condylar full-thickness chondral defect (not shown) is easily identified on the dark fluid three-dimensional gradient-recalled echo sagittal image due to the large contrast difference between the high signal of cartilage fragment and the dark fluid. (b) Two-dimensional proton-density fast spin-echo sagittal image also demonstrates the fragment (arrow), but it is slightly less distinct because it is partially averaged with adjacent synovial proliferation of similar intensity and is somewhat less distinct in bright fluid.

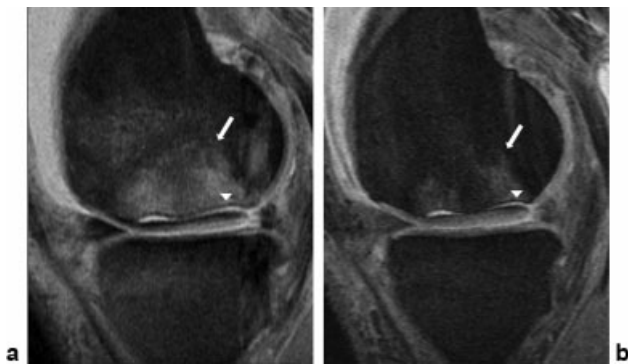


Fig. 2 A large osteochondral lesion of the medial femoral condyle with bright fluid (white arrowhead) undercutting an intra-articular osteochondral fragment is well visualized (a) on the sagittal fat-saturated two-dimensional (2D) proton-density (PD) fast spin-echo (FSE) and (b) on the bright fluid three-dimensional (3D) gradient-recalled echo (GRE) double-echo steady-state sequences. Associated bone marrow edema (white arrow) is prominent (a) on the 2D PD FSE image but is less conspicuous (b) on the 3D GRE image.

with inherently higher signal than lower strength MRI systems and can therefore better compensate for signal loss or noise. The reported diagnostic performance of 3D FSE, including for cartilage, has been lower on 1.5-T systems than on 3-T systems.^{1,2,4,5,35}

Three-dimensional FSE sequences can be performed using a variety of image contrast techniques. Intermediate-weighted 3D FSE acquisitions can produce images with signal properties similar to those seen with the PD-weighted sequences typically used for 2D knee MRI. This allows for the use of 3D FSE sequences to assess not only cartilage but also structures such as bone marrow, menisci, tendons, and ligaments while still providing high-resolution isotropic or near-isotropic evaluation. As a result, 3D FSE sequences provide a more global joint assessment, an important advantage over 3D GRE sequences.^{1,2} These isotropic 3D FSE sequences also maintain the ability to minimize partial volume averaging while allowing MPRs to be performed (► Fig. 3).

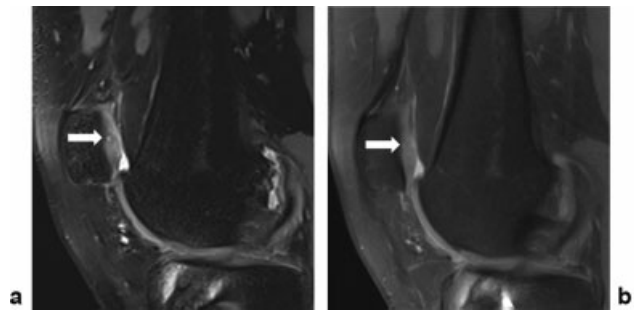


Fig. 3 A high-grade patellar chondral fissure (arrow) is well visualized (a) on the fat-saturated sagittal three-dimensional fast spin-echo (FSE) sequence (0.6-mm slice thickness) but is not as well visualized on (b) a corollary two-dimensional proton-density FSE sequence (2.8-mm slice thickness) because of partial volume averaging.

Many studies have therefore evaluated the feasibility of replacing traditional multiplanar 2D sequences with a single 3D FSE acquisition for a faster diagnostic global knee joint assessment.^{4-7,36,37} Although most of these studies have shown that the diagnostic abilities of 3D FSE sequences are for the most part similar to those of 2D FSE sequences, we are not aware of any large institution that has replaced its 2D protocol with a single 3D FSE sequence. Rather, evolving MRI acceleration techniques for both 2D and 3D sequences now allow for acquisition of both multiplanar 2D sequences and high-resolution 3D FSE knee MRI sequences in a feasible time. At our institution, our routine knee protocol on 3-T scanners consists of five 2D FSE sequences and a 3D FSE sequence obtained using parallel imaging in a total acquisition time of ~ 10 minutes.

Compositional Knee MRI

Compositional cartilage imaging is one of the most studied applications of 3D MRI techniques in the knee.^{9,17,19,38} Most often performed in the research setting, compositional imaging involves creating a cartilage parameter map based on measurements of specific MR parameters over time that can then be used (depending on the compositional sequence employed) to infer the intrinsic biochemical properties of the articular cartilage, including water content, glycosaminoglycan and proteoglycan content, and type II collagen network integrity. Essentially all compositional techniques, including T2* maps, T1ρ, delayed gadolinium-enhanced MRI of cartilage (dGEMRIC), diffusion-weighted imaging (DWI), T2, and sodium 23 MRI, have been investigated with 3D spatially encoded acquisitions.^{9,17,19}

Typically, a high-resolution isotropic 3D GRE or 3D FSE sequence is obtained alongside a compositional map sequence, which can be a 3D or 2D spatially encoded acquisition.^{23,39,40} Cartilage segmentation is then performed, usually using the high-resolution isotropic 3D sequence, and the segmentation is registered to the compositional map that typically consists of thicker slices because of SNR or acquisition limitations. For T2* mapping, however, high-resolution isotropic maps can often be obtained.^{9,41} Of these compositional techniques, only T2, T2*, and T1 (dGEMRIC) maps are currently available for clinical systems. The long acquisition times of these compositional

sequences and the manual or semi-manual cartilage segmentation required have prevented more widespread clinical adoption of these techniques. However, new accelerated imaging techniques and automated cartilage segmentation using machine learning show promise for future clinical integration.

Metal Artifact Suppression

Another rapidly expanding clinical application for these 3D encoded techniques is the reduction of metal artifacts when scanning a patient with hardware such as knee arthroplasties. Advanced metal artifact reduction techniques use 3D spatially encoded MRI techniques to reduce through-plane artifact. For instance, the multi-acquisition variable-resonance image combination (MAVRIC) sequence directly uses 3D excitation and 3D readout pulses.^{11,26} Slice encoding for metal artifact correction (SEMAC), in contrast, uses a 2D excitation pulse with a 3D readout pulse.¹¹ These sequences have been shown to reduce hardware artifact markedly when compared with traditional techniques to reduce metal artifact (e.g., using FSE sequences and increasing receiver bandwidth). Given the increased magnetization of hardware at higher field strengths, these sequences are most effective when employed on 1.5-T systems rather than on 3-T systems. The long acquisition time required is the primary limitation of this technique, although new acceleration techniques using compressed sensing can substantially reduce imaging times.²⁶

MRI Neurography

Three-dimensional MRI techniques can also be useful for assessing peripheral nerves, including nerves around the knee.^{14,15,42} T2-weighted isotropic 3D FSE MRI sequences with various fat-suppression techniques are increasingly being incorporated into clinical peripheral neurography protocols. Although not specifically optimized for neurography, isotropic 3D FSE sequences commonly included in clinical knee MRI protocols are often acquired with similar fluid-sensitive weighting and fat suppression that allow for high-resolution assessment of the nerves and the ability to perform MPRs (→ Fig. 4). Vessel signal suppression is a technique often used in MRI neurography sequences to isolate signal from the nerves within the neurovascular bundle.⁴³

Although 3D FSE sequences intrinsically suppress signal in high-flow velocity vessels, such as arteries, due to low refocusing pulses that are sensitive to motion, the venous signal usually remains predominantly bright and may obscure or confound nerve assessment. Dedicated 3D FSE peripheral neurography protocols use fat-suppressed T2-weighted sequences with dedicated pulse techniques or T1 shortening intravenous gadolinium contrast to further suppress blood signal from veins.^{13,42} Three-dimensional DWI techniques can also be used to suppress the vascular signal and enhance the nerve signal, allowing these techniques to be employed for isotropic peripheral neurography protocols; however, these DWI techniques are limited by sensitivity to field inhomogeneities and motion.⁴³ Diffusion tensor imaging, which uses anisotropy of diffusion that occurs along a nerve to visualize the course of the nerve

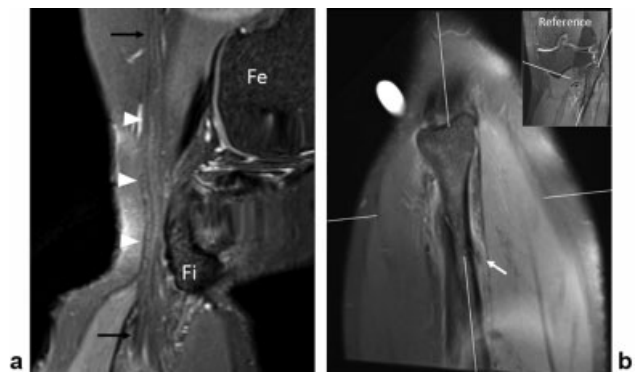


Fig. 4 (a) For a patient with peroneal nerve symptoms after an injury, the entire course of the common peroneal nerve is visualized on a single image with a curved multiplanar reconstruction (MPR) using a three-dimensional fast spin-echo sequence acquired as part of a standard knee protocol, demonstrating segmental nerve fascicle enlargement and increased signal (white arrowheads) proximal to the fibula relative to the normal signal and caliber of the more proximal and distal portion of the nerve (black arrows), consistent with neuritis. (b) The subacute healing nondisplaced proximal fibular fracture (white arrow) is also well depicted on a thick nonorthogonal MPR along the long axis of the fibula, oblique to the routine sagittal plane; the fracture was occult on radiographs at the time of the trauma. A reference image (top right corner) is provided to demonstrate the referenced nonorthogonal planes used to create an optimized MPR. Fe, femur; Fi, fibula.

(fiber tractography), is another 3D technique that can be used for MR neurography, but this technique requires considerable optimization and postprocessing time to yield productive images, thus limiting its clinical use (→ Fig. 5).

Advantages

Decreased Partial Volume Averaging

A primary advantage of high-resolution 3D MRI when compared with 2D FSE MRI is a reduction in partial volume averaging artifacts in the slice direction.^{3,28} Isotropic or near-isotropic resolution 3D sequences have cube-shaped voxels with a slice thickness that is nearly or completely equivalent to the in-plane resolution. Two-dimensional sequences, in contrast, have rectangular-shaped voxels with a slice thickness that is typically five to nine times greater in the slice direction than the in-plane resolution. These larger voxels result in a predisposition to partial volume averaging of MR signal along the slice direction. Although this averaging has the benefit of increasing SNR in thicker 2D images, it can also blend together different anatomical structures and signals that can obscure potentially clinically relevant pathology or artifactually create the appearance of pathology in otherwise normal anatomy. This is particularly true for small structures with curved or anatomically oblique orientations, such as articular cartilage or menisci in the knee.¹⁶

Morphological assessment of articular cartilage is the most common reason for including a 3D acquisition in knee MRI examinations in both the clinical and research settings. Both 3D GRE and 3D FSE sequences can be helpful in evaluating articular cartilage, due in large part to decreased partial volume averaging. Numerous studies have evaluated cartilage assessment using a variety of 3D FSE sequences

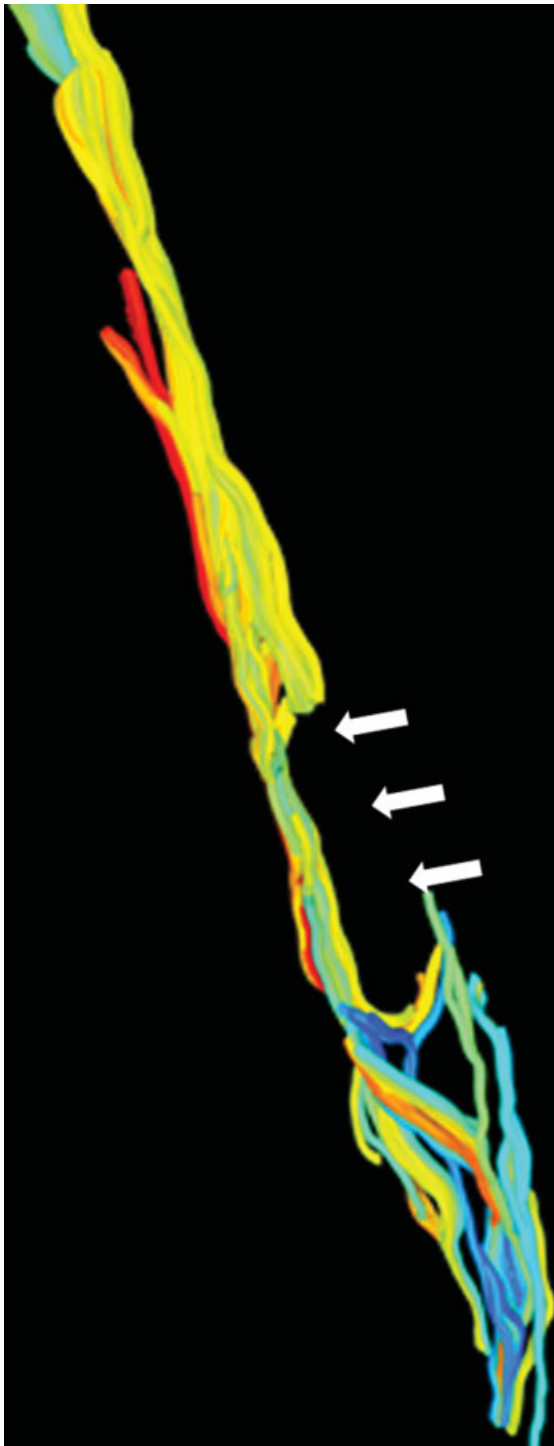


Fig. 5 Rendered magnetic resonance diffusion tensor imaging of the sciatic nerve demonstrates and differentiates between disrupted nerve fibers (arrows) and intact nerve fibers in a patient with a gunshot injury of the thigh.

from different vendors, and a comprehensive meta-analysis of these studies in 2018 found that 3D FSE sequences were more sensitive and specific than multiplanar 2D FSE protocols for cartilage assessment.¹ Although 3D FSE sequences have advantages over 3D GRE sequences for cartilage assessment, the contrast difference between articular cartilage and fluid, especially on bright fluid GRE sequences, was shown to

increase sensitivity for detecting superficial partial-thickness cartilage lesions.^{8,29}

Three-dimensional GRE sequences have also been found to increase specificity when used as a supplement to 2D FSE sequences. However, 3D GRE sequences have lower sensitivity for the detection of cartilage lesions overall when compared with 2D FSE sequences alone, in part because of poor conspicuity of subchondral marrow signal changes (an important secondary marker of adjacent chondral pathology) (**Fig. 2**).^{1,8}

Decreased partial volume averaging can also be a benefit when evaluating other structures in the knee, such as menisci. Most studies have found that 3D FSE and 2D sequences offer comparable diagnostic accuracy for detecting meniscus pathology.² Thus 3D imaging can be particularly helpful in detecting small radial tears that can be obscured by partial volume averaging on 2D images but are more apparent on 3D images.^{3,25} Similarly, 3D imaging can be helpful in diagnosing normal meniscal flounce, which can mimic a tear on 2D images because of partial volume averaging. At our institution, we routinely obtain a high-resolution 3D FSE sequence (when available) or a 3D GRE sequence that is typically bright fluid to assess articular cartilage and menisci.

Multiplanar Reconstructions

Another important advantage of high-resolution isotropic 3D knee MRI is the ability to create MPRs in any imaging plane without a substantial loss of in-plane image resolution, thus obviating the need to acquire multiple sequences in different imaging planes, as required with 2D imaging. These 3D sequences can be used to either replace 2D multiplanar sequences or to supplement them. With the advent of 3D FSE sequences and their ability to provide contrast similar to that of 2D FSE sequences, multiple studies have evaluated knee MRI protocols consisting of only one or two 3D FSE sequences.^{4,36} The main advantage of such a protocol is that it can substantially reduce acquisition time when compared with standard protocols consisting of multiple 2D FSE sequences in the axial, coronal, and sagittal planes. Using isotropic 3D acquisitions would also eliminate difficulties or the need for repeat acquisitions due to incorrect imaging plane prescriptions by technologists, a problem especially common in the setting of oblique or radial planes.

Although studies have shown that the diagnostic performance for this type of 3D FSE protocol is similar to that of standard 2D protocols, we are unaware of any institution that has replaced its 2D sequences in favor of one or two 3D sequences with MPR reformations, likely because of the disadvantages associated with a 3D protocol, discussed later. Instead, 3D MRI with MPRs more commonly supplement 2D sequences obtained in standard planes. One of the most common uses of 3D MPRs is to generate images along non-orthogonal planes to better depict anatomical structures coursing in oblique or radial orientations that otherwise would necessitate additional 2D acquisitions.¹⁶ These reconstructions can be created with any desired slice thickness to optimize the balance of SNR lost from thinner slices with the partial volume averaging artifacts that result from thicker slices. Most clinical picture archive and communication

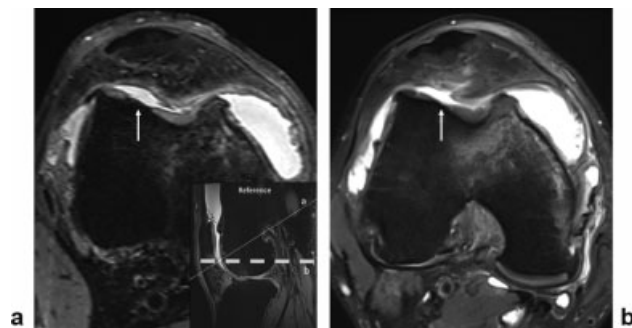


Fig. 6 (a) A moderate-sized full-thickness chondral fissure/defect in the lateral trochlea (arrow) is well visualized and characterized on a thin three-dimensional (3D) fast spin-echo (FSE) axial oblique multiplanar reconstruction (MPR) due to optimal orientation of the imaging plane perpendicular to the curved articular surface of the trochlea at the site of the defect. (b) The same lesion (arrow) is suboptimally characterized on the two-dimensional (2D) T2-weighted FSE standard axial sequence due to partial volume averaging with adjacent cartilage as a result of thicker slices and oblique orientation of the imaging plane through the defect. A sagittal reference image (a, lower right corner) demonstrates the thinner 3D MPR plane (thin line) and the thicker standard axial 2D plane (thick dashed line).

systems offer the radiologist the option to manipulate and view the 3D data set interactively with MPRs to optimally display and highlight pathology for the particular study at hand without the need to explicitly export additional images.

For articular cartilage, nonstandard planes can be of particular utility in analyses of the trochlea and posterior femoral condyles. Studies have demonstrated that 1-mm-thick radial reformats of 3D FSE acquisitions for evaluation of the curved surface of the femoral condyles can improve the accuracy of articular cartilage evaluation when compared with 2D sequences and orthogonal 3D FSE reconstructions (→ Fig. 6).¹⁶

The menisci can be similarly assessed with nonorthogonal MPRs. Radial reconstructions of 3D FSE sequences perpendicular to the curved course of the menisci can supplement assessment and characterization of meniscal tears and meniscal extrusion, particularly in regions that are suboptimally assessed in standard imaging planes, such as the root or the junctions of the body with the posterior and anterior horns (→ Fig. 7).^{3,25} Additionally, some tear types, particularly radial tears, can be best appreciated on 3D isotropic MPRs oriented axially to the meniscal curvature that may not match the plane of orthogonal 2D axial images.

Three-dimensional MPRs can also help assess ligaments and tendons of the knee that often course in nonorthogonal planes. For example, some institutions obtain oblique sagittal images along the course of the anterior cruciate ligament to improve visualization of the ligament; however, this protocol is not ideal for evaluating the femoral condyle cartilage, thereby necessitating the acquisition of two 2D sagittal sequences. With a 3D FSE sequence, both sagittal oblique and axial oblique MPR images along the course of the anterior cruciate ligament can be generated if needed. Similarly, MPRs or curved reconstructions along the long or short axis of a coursing tendon can be used to optimize visualization of tendon pathology.

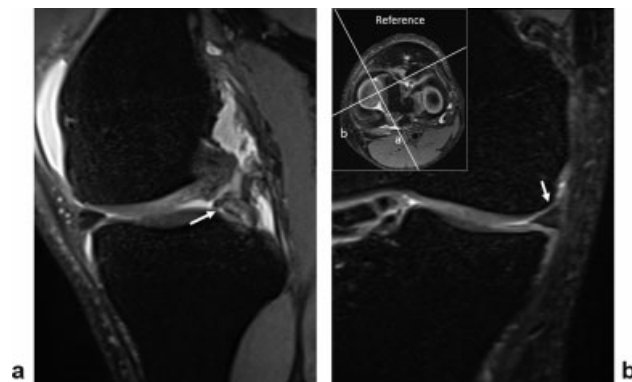


Fig. 7 Radial multiplanar reconstructions (MPRs) perpendicular to the entire semicircular course of the menisci generated using a three-dimensional (3D) viewer tool available on the picture archive and communication system from a 3D fast spin-echo (FSE) acquisition demonstrates (a) a posterior root meniscus tear (arrow) with (b) early meniscal extrusion (arrow) optimally compared with standard orthogonal coronal and sagittal two-dimensional planes (not shown). A reference image (b, top left corner) is provided to demonstrate the referenced nonorthogonal planes used to create the optimized radial MPRs.

At our institution, we acquire 3D FSE or GRE sequences with submillimeter voxels in the sagittal plane and create 1-mm-thick straight sagittal, straight coronal, and oblique axial reformats to balance the improved resolution of the thinner slices with the improved SNR of the thicker slices. Axial oblique images oriented perpendicular to the trochlea simultaneously improve the visualization of the trochlear cartilage, the anterior cruciate ligament, and the meniscal roots that are all oriented along a similar plane.

Segmentation and Quantitative Assessment

Isotropic 3D morphological sequences are also well suited for segmentation, particularly for volumetric analyses or surface rendering.^{23,32,39,44,45} Additionally, isotropic resolution for segmentation minimizes registration errors and eliminates the need to segment the same anatomy in multiple planes.

The high out-of-plane resolution of isotropic 3D FSE or GRE sequences is particularly well suited for segmentation of small or thin anatomical structures, such as articular cartilage, given the many curved surfaces of the knee prone to partial volume averaging. Segmentation not only allows for measurement of cartilage thickness and volume but is also a prerequisite step for compositional analysis of articular cartilage.³⁹ As such, these isotropic sequences are often used alongside 2D or 3D spatially encoded compositional map acquisitions. Although compositional articular cartilage sequences are currently not used in most clinical environments because of the time-consuming process required to segment articular cartilage, the development of fully automated segmentation techniques is bringing these sequences closer to implementation in routine clinical practice.^{23,39}

Along the same lines, segmentation and surface rendering of bones using 3D imaging are increasingly being used for preoperative planning.³ Traditionally, computed tomography (CT) was used to generate bone models. Recent studies, however, have shown that several isotropic or near-isotropic

3D MRI sequences can be used instead of CT. Using these 3D MRI sequences not only eliminates the need to perform an additional study but also the need to expose patients to ionizing radiation. At our institution, for example, we have found that a 3D two-point Dixon sequence is interchangeable with CT for preoperative planning for femoroacetabular surgery in the hip, although we currently do not explicitly use 3D MRI for this purpose in the knee. Nonetheless, optimized MPRs can allow for excellent diagnostic assessment of osseous structures, particularly with 3D FSE sequences for obliquely oriented anatomy (► Fig. 4).

Metal Artifact Reduction

Three-dimensional MRI sequences can also be used to reduce metal artifact.¹¹ Although traditional 2D FSE optimization techniques, such as increasing receiver bandwidth, are helpful in reducing in-plane distortions caused by metal hardware, they do not correct for through-plane distortions along the slice direction. New advanced metal artifact reduction sequences, such as MAVRIC and SEMAC, in contrast, use 3D spatial encoding techniques to correct not only for in-plane distortions but also for through-plane distortions. The use of these 3D MRI sequences for metal artifact reduction was shown to improve the detection of hardware complications such as osteolysis, periprosthetic fractures, fluid collections, and soft tissue masses. These sequences can also be helpful for assessing intra-articular structures, such as articular cartilage, menisci, and ligaments, that would otherwise be obscured by metal artifact in the setting of a unicompartmental knee arthroplasty (► Fig. 8). These 3D metal artifact reduction sequences, now available through multiple vendors, are replacing standard 2D FSE sequences for imaging joints in patients with metal hardware. At our institution, we routinely use SEMAC sequences instead of standard 2D sequences when imaging patients with knee arthroplasties or metal hardware around the knee.

Imaging of Nerves

The high spatial resolution of isotropic 3D sequences is also beneficial when evaluating peripheral nerves that are typically small in caliber and course in nonorthogonal planes. Isotropic

3D FSE sequences have shown particular promise for the evaluation of nerves (► Fig. 4). Three-dimensional FSE sequences, despite being optimized for the evaluation of articular cartilage, ligaments, and tendons, are similar to 3D FSE protocols optimized for dedicated MR neurography techniques used to evaluate peripheral nerves. Dedicated 3D MR neurography sequences, such as diffusion-weighted reversed fast imaging with steady-state precession, can suppress signal from vessels to highlight the nerves and provide excellent assessment of peripheral nerves around the knee.^{13,42} Regardless of the type of 3D sequence used, optimized MPRs can be of use for assessing the sciatic nerve and branches, as well as the common peroneal nerve and branches along the curved course around the fibular head. These MPRs can also be used to create thicker maximum intensity projection slabs to visualize a large segment of a nerve on a single image. At our institution, we use a near-isotropic 3D FSE sequence as part of our MR neurography protocol; from this sequence, nonorthogonal and curved MPRs can be generated along the course of the nerve of interest.

Limitations

Time Limitations

One of the biggest barriers to incorporating 3D knee MRI sequences into routine clinical practice is the long acquisition time.^{10,30} This is particularly true in the case of high-resolution submillimeter isotropic or near-isotropic 3D FSE acquisitions that can take >8 minutes to acquire. This is a substantially longer acquisition time than required for a single 2D FSE acquisition. Because 3D sequences are currently most often used to augment rather than replace 2D sequences, the incorporation of a 3D sequence into the routine protocol results in added imaging time. Long acquisition times can also increase the potential for motion artifacts, and it may be problematic if repeat acquisition is necessary. As a result, many practices do not routinely obtain a 3D sequence as part of the knee protocol. Emerging techniques to accelerate 3D image acquisition hold the promise to lower this barrier; these techniques are discussed later.

MPRs also require additional postprocessing time either by the technologist or by the radiologist. Additionally, although thinner slices result in decreased volume averaging, they also result in many more images that need interpretation. The image count can increase from twofold to fivefold, depending on the thickness of the MPR images and the number of reconstruction planes generated, which can increase interpretation time.

Contrast Weighting and Single Acquisition

One of the main advantages of standard multiple-plane 2D knee MRI protocols is that they include sequences with different image contrast weightings. Most protocols include sequences with PD weighting for optimized evaluation of menisci and cartilage, T2 weighting for optimized evaluation of tendons and ligaments, and T1 weighting for optimized evaluation of marrow. Along the same lines, most standard 2D protocols include both fat-saturated sequences to

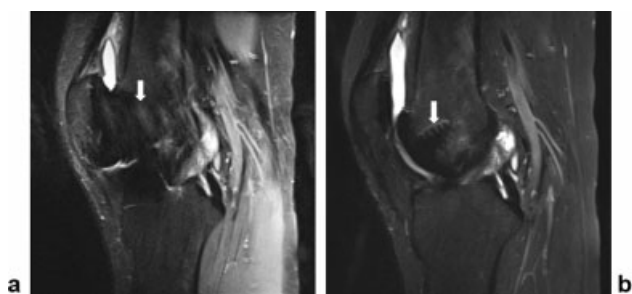


Fig. 8 (a) Metal artifact from a patellofemoral compartment arthroplasty obscures visualization of the metal–bone interface (arrow) of the trochlear implant on a two-dimensional high-bandwidth short tau inversion recovery (STIR) sagittal image. (b) A corollary sagittal STIR image from an advanced three-dimensional metal artifact reduction sequence using slice encoding for metal artifact correction (SEMAC) allows clear visualization of the metal–bone interface (arrow) due to reduction of through-plane metal artifact.

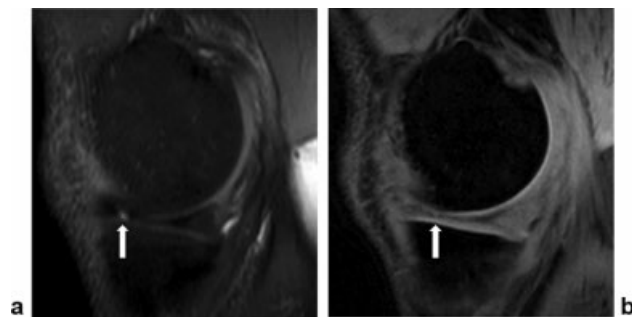


Fig. 9 (a) Sagittal proton-density-weighted two-dimensional sequence clearly demonstrates a radial tear (arrow) in the anterior inner margin of the medial meniscus. (b) This tear (arrow) is not well visualized on a corollary three-dimensional gradient-recalled echo sequence because of poor meniscus–fluid contrast.

increase conspicuity of edema and non-fat-saturated sequences to improve anatomical detail.

In contrast, a 3D sequence with MPRs is limited to a single contrast-weighting and fat-suppression technique. Although 3D FSE sequences can reproduce PD weighting, T2 weighting, and T1 weighting, the use of just one contrast-weighting technique limits the ability of this sequence to optimally evaluate all of the structures in the knee. Furthermore, in the case of 3D GRE sequences, the contrast-weighting technique is dissimilar to PD-weighted, T2-weighted, and T1-weighted sequences in that there is more T2* dependence, and so the use of this sequence is limited for global joint assessment. Similarly, images with fat saturation and without fat saturation offer distinct advantages and disadvantages, depending on the pathology. Although most studies have found that a single 3D FSE sequence protocol with MPRs has diagnostic performance similar to that of a standard multiple-plane 2D protocol, some studies have shown decreased sensitivity of both 3D GRE sequences and, in a few studies, 3D FSE sequences for detecting meniscal tears, likely related to suboptimal contrast weighting (► Fig. 9).^{2,5,37}

Although a single 3D sequence protocol may therefore not be the answer to replace 2D sequences, studies showed it may be more feasible to use a protocol with two accelerated 3D FSE sequences in lieu of 2D sequences.³⁶ At this time, however, we are not aware of any large practice that has replaced its standard knee protocol with a protocol consisting only of 3D sequences.

Diagnostic and Quality Limitations of Isotropic 3D MRI

Apart from imaging time and contrast weighting, there are other diagnostic limitations to isotropic 3D knee MRI imaging for both GRE and FSE sequences. Although the out-of-plane spatial resolution of 3D sequences is much higher than that of 2D sequences, the in-plane resolution of 3D sequences is usually slightly lower than for 2D sequences.^{4,5} Additionally, the smaller voxels, due to thinner slices in 3D acquisitions, result in overall decreased signal in each voxel that reduces SNR. SNR is often further reduced due to undersampling acceleration techniques that are often required to obtain 3D FSE sequences within a feasible time. Although these limitations can be partially overcome by using 3-T systems and by

creating MPRs with thicknesses that optimize the balance between SNR and partial volume averaging, the image quality of 2D sequences is often still superior to that of 3D sequences.¹²

Additionally, for 3D GRE sequences, susceptibility artifact from the absence of a refocusing pulse limits the ability of these sequences to evaluate areas prone to this artifact, such as in the presence of hardware or in the bone marrow (► Fig. 2).³² Decreased bone marrow edema signal on GRE images not only limits the ability of these sequences to identify bone pathology but also affects their ability to evaluate articular cartilage. The decreased conspicuity of subtle subchondral marrow signal changes that can help identify overlying cartilage abnormalities has been hypothesized as the reason why 3D GRE sequences are less sensitive for identifying cartilage lesions than 2D sequences, despite having thinner slices with less partial volume averaging.³ Short echo times with 3D GRE sequences can also result in magic angle artifacts when evaluating obliquely coursing structures such as tendons.

Because of these limitations with 3D GRE sequences, most practices have replaced 3D GRE sequences with 3D FSE sequences when available. However, 3D FSE sequences also have limitations, including image blurring, caused by the long echo train lengths and undersampling techniques used to reduce acquisition time.³² Meta-analyses showed that only articular cartilage evaluation is improved with the use of 3D FSE sequences, whereas evaluations of other structures, such as menisci, ligaments, and bone marrow, remain comparable with evaluations with 2D sequences.^{1,2} Some studies have demonstrated marginally better performance for some meniscal tear subtypes with multiplanar 2D sequences than with 3D FSE sequences, although these findings have not been consistent and have not demonstrated any measurable differences in meta-analyses.^{5,37} Interestingly, it remains unclear whether 3D FSE sequences reconstructed with thicker slices (similar to those used in 2D sequences) also have a diagnostic performance similar to that of 2D sequences. As a result of these limitations, 3D FSE sequences are typically used in addition to 2D FSE rather than as a replacement.

Emerging Techniques

Recent advances in MRI acceleration technologies and techniques have been instrumental to the advancement of 3D knee MRI. Compared with 2D acquisition, 3D acquisition is better suited for acceleration techniques such as parallel imaging and compressed sensing.^{12,25,27,38} This has influenced the growth and adoption of 3D FSE sequences over the past decade, and more recently, this has expanded to other applications such as compressed sensing metal artifact reduction sequences.²⁶ Broadly, all acceleration techniques rely on undersampling of data that results in a decrease in SNR and an increase in artifacts. The primary challenge in the development of accelerated sequences is maintaining diagnostic image quality. As in 2D imaging, sequence optimization in 3D imaging often depends on identifying parameters that balance the acquisition time, image resolution, and SNR to suit the clinical needs. As such, although acceleration techniques are often considered

successful when continuing to yield diagnostic images with shorter acquisition times, they can also ultimately be used to obtain images with similar scan times but with more optimized parameters, such as higher resolution.

The most widely used acceleration technique currently is parallel imaging, a key component of 3D FSE sequences.¹² Parallel imaging reduces acquisition time by decreasing the number of phase-encoding steps acquired and using the spatial sensitivity of multichannel surface coils to unfold the resultant aliased signal.³⁸ This unfolding can be performed in the image domain, termed sensitivity encoding, or in the k-space domain, termed generalized autocalibrating partial parallel acquisition (GRAPPA). Although both techniques have their unique advantages and disadvantages, they are largely interchangeable. One of the main advantages of the parallel imaging technique is that it is applicable to a broad range of acquisition types, including FSE and GRE sequences, 2D and 3D acquisitions, and compositional imaging techniques. The biggest drawback of this technique is that it results in a reduction in the SNR by a factor roughly the square root of the acceleration factor. To minimize the effect of this SNR loss on image quality, it is highly beneficial to start with high SNR images, such as those obtained on 3-T systems. Even at 3 T, however, the loss in SNR usually prohibits acquisition acceleration beyond a factor of 2.

Submillimeter isotropic 3D FSE sequences using parallel imaging with an acceleration factor of 2 can have acquisition times too long for clinical protocols, sometimes requiring ≥ 8 minutes. More recently, however, a parallel imaging technique with an acceleration factor of 4 became available for 3D FSE techniques, termed CAIPIRINHA (Controlled Aliasing in Parallel Imaging Results in Higher Acceleration).⁴⁶ CAIPIRINHA takes advantage of the fact that phase encoding occurs in two directions in a 3D acquisition, skipping phase-encoding steps in both directions while minimizing the loss in SNR that typically occurs with fourfold acceleration by incorporating a phase shift to the k-space sampling. With CAIPIRINHA, acquisition times can be reduced to 5 minutes for a submillimeter isotropic 3D FSE acquisition with diagnostic image quality. This shorter acquisition time provides the ability to obtain multiple 3D FSE sequences with different contrast weightings and fat saturation techniques in a clinically feasible time, thus partially addressing the limitations of the single-sequence 3D protocol discussed earlier. A 2018 study evaluated a 10-minute knee protocol consisting of two 3D FSE CAIPIRINHA sequences, one with fat saturation and one without, and demonstrated diagnostic performance comparable with that of a multiplanar 2D protocol with an acquisition time twice as long for global joint assessment at both 1.5 T and 3 T.³⁶ At our institution, although we continue to use a 3D FSE sequence with standard time optimizations and an acceleration factor of 2 for our clinical cases, we have begun evaluating a CAIPIRINHA 3D FSE sequence with an acceleration factor of 4 in some research studies.

Compressed sensing is another undersampling technique that has been successfully applied to 3D FSE sequences and metal artifact reduction sequences with acceleration factors

> 2 . This technique is based on the same principles used in digital image compression algorithms that exploit inherent sparsity (lack of information) on mathematical transformations of image data to reduce digital image size while maintaining perceived quality. Compressed sensing uses a similar process in reverse, undersampling k-space in a pseudo-random manner while preserving the essential data in the center of k-space, transforming the k-space data into a domain where there is data sparsity, and then iteratively reconstructing the data back into the image domain.¹² Like parallel imaging techniques, compressed sensing techniques are more suited for 3D sequences that inherently have greater data sparsity than 2D sequences; this is especially the case with metal artifact reduction sequences such as SEMAC. Compressed sensing 3D FSE sequences have demonstrated SNR and diagnostic image quality comparable with the SNR and image quality of standard 3D FSE sequences in the knee, although some studies have noted image blurring as a diagnostic issue with compressed sensing.^{12,25} Compressed sensing SEMAC sequences can substantially reduce imaging time while still providing metal artifact reduction similar to that provided by standard SEMAC sequences.²⁶ At our institution, when imaging patients with arthroplasties, we have begun using compressed sensing SEMAC sequences when available, resulting in a reduction in imaging times.

Compressed sensing acceleration can also be applied to nonmorphological sequences, such as some compositional cartilage imaging techniques.⁴⁷ Compositional cartilage imaging sequences, such as T2 mapping and T1 ρ , traditionally require long acquisition times (> 10 minutes), which has been a barrier to the incorporation of these techniques into routine clinical practice. At our institution, we developed a compressed sensing 3D T1 ρ sequence with up to eightfold acceleration that permits a whole-knee relaxometry map acquisition in 3 to 4 minutes (**Fig. 10**). Like other acceleration techniques, compressed sensing is not without its limitations. The iterative reconstruction required for compressed sensing increases computational hardware processing requirements and time, and the undersampling and iterative reconstruction methods can lead to loss of details and edge sharpness.¹²

Acceleration techniques using artificial intelligence (AI) algorithms are also on the horizon, and these techniques may be the most promising of all. Two recent studies demonstrated that deep learning acceleration can be used successfully for knee MRIs with acceleration factors ≥ 4 .^{21,22} In both of these studies, the deep learning algorithms were trained on retrospectively undersampled k-space from 2D sequences using different types of convolutional neural networks. For AI acceleration techniques, although model training is an iterative process that can be time intensive and computationally demanding, once the model is fully trained, image reconstruction is fast and can be performed without the need for special reconstruction hardware. Another advantage of AI acceleration is that it may be possible to create highly accelerated images without the loss in image quality seen with the other imaging techniques. In fact, the AI-accelerated images were actually preferred over the standard images in one of these recent studies.²¹ The main drawback of AI acceleration, as with other AI applications, is that

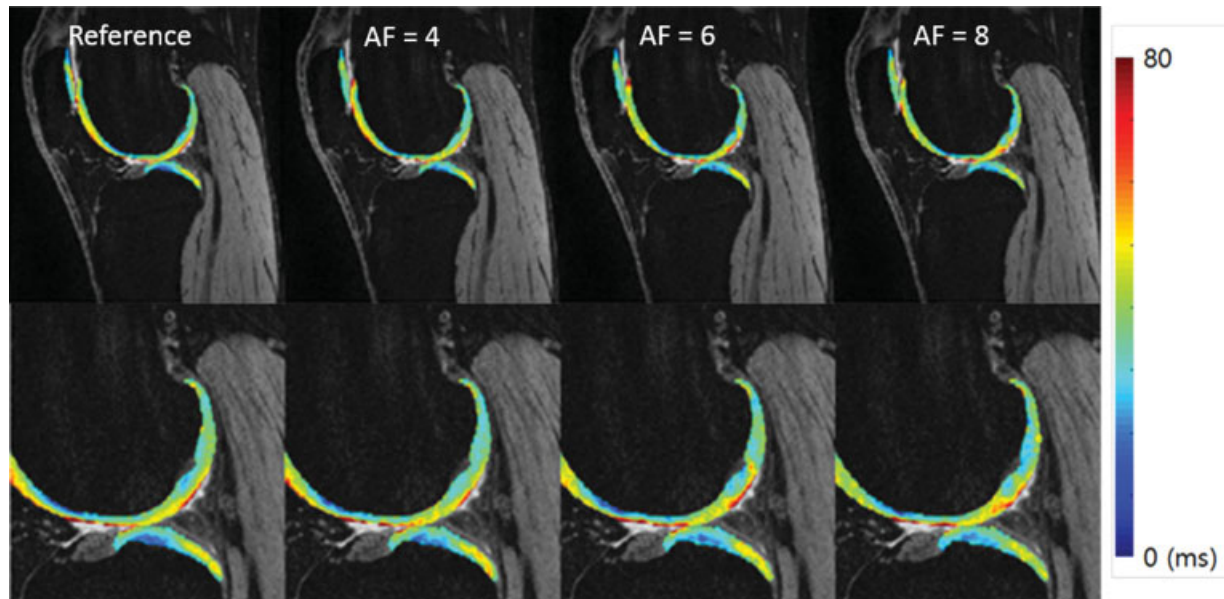


Fig. 10 Compressed sensing can be used to decrease acquisition time of a three-dimensional T1 ρ sequence without a clinically significant difference in accuracy. Reference acquisition using parallel imaging with an acceleration factor (AF) = 2 and a time of acquisition (TA) = 13:43 can be reduced to TA = 6:37 (AF = 4), TA = 4:24 (AF = 6), and TA = 3:18 (AF = 8), with < 4% difference in the average coefficients of variation between reference and accelerated sequences for all AFs. Top: whole image within field of view; bottom: zoomed-in images.

a large amount of training data are needed, and the methodology behind the algorithm is a black box. To our knowledge, no 3D AI acceleration sequences are currently available for clinical use. However, we have developed a combined T1 ρ and T2 map sequence with acquisition AI acceleration factors as high as 12, resulting in acquisition times approaching 1 minute and with quantitative values comparable with those of a fully sampled multiecho sequence (\rightarrow Fig. 11).

Thus far, we have primarily focused on the advantages and limitations of 3D MRI techniques for morphological imaging, but 3D MRI techniques are also an integral part of quantitative MRI protocols, such as compositional cartilage imaging. Aside from the long acquisition times required to obtain these compositional sequences, another barrier to the adoption of these techniques into routine clinical practice is the postprocessing required that is time consuming and traditionally was

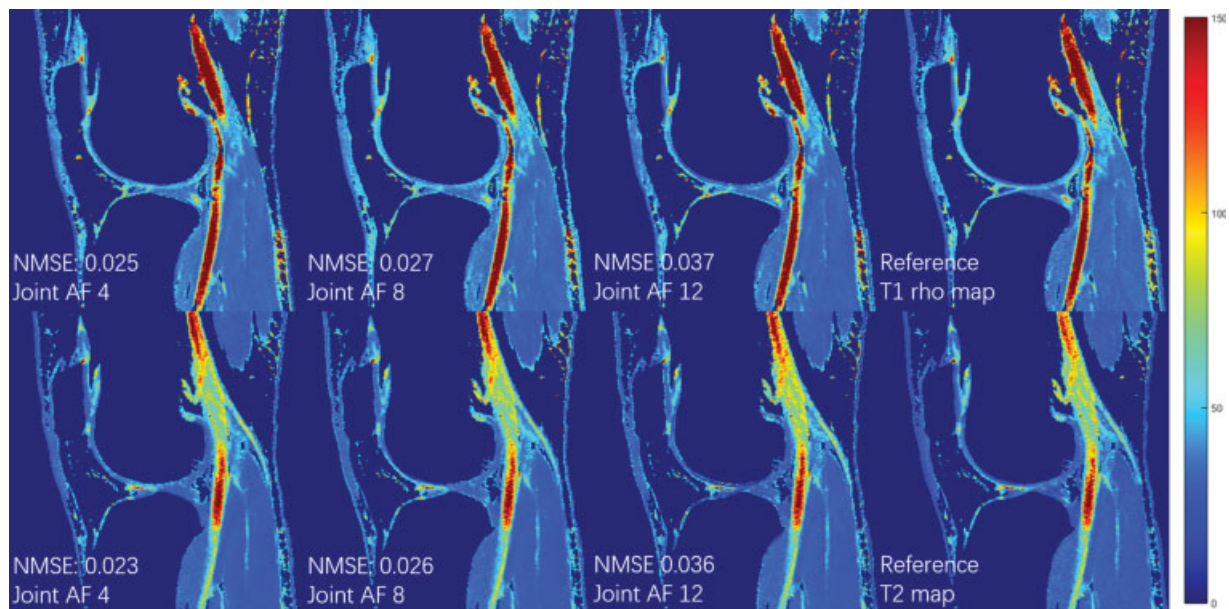


Fig. 11 A deep learning algorithm can be used to accelerate a combined T1 ρ and T2 three-dimensional sequence without a clinically significant difference in accuracy. T1 ρ (top) and T2 (bottom) maps with acceleration factors (AFs) of 4, 8, and 12 were obtained from retrospective undersampling of the reference T1 ρ and T2 maps (acquisition time = 13:43) from eight fully sampled echoes. The deep network exploits both the spatial correlation among pixels and the temporal correlation between the selected echoes while algorithmically learning the complicated nonlinear relationship between the subsampled T1 ρ /T2-weighted images and the T1 ρ /T2 maps. NMSE, normalized means squared error.

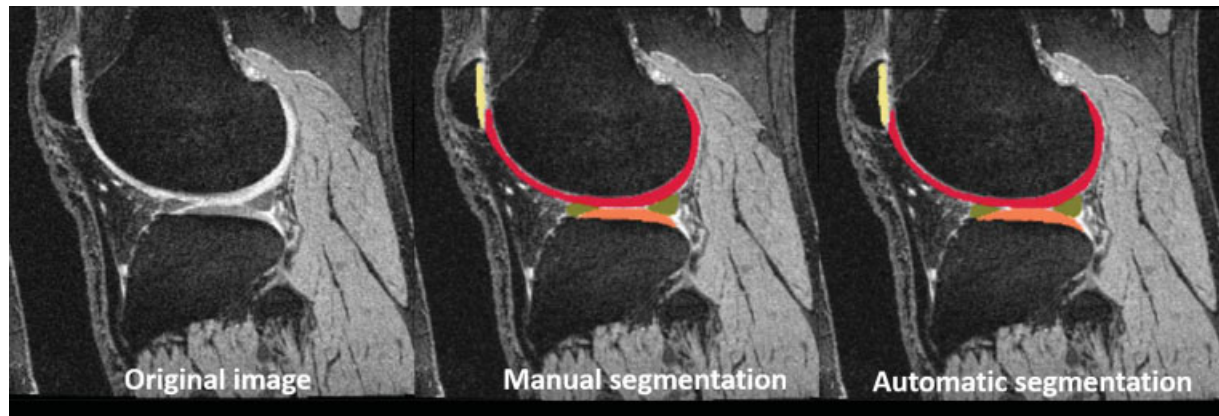


Fig. 12 Fully automatic segmentation of cartilage and meniscus using a deep learning generative adversarial network (Unet-cGAN)-based model and three-dimensional gradient-recalled echo double-echo steady-state images from the Osteoarthritis Initiative, with accuracy comparable with that seen with manual segmentation.

performed either entirely manually or semi-manually. As a result, these sequences have been relegated almost entirely to the research setting. Recent studies, however, showed that the postprocessing needed for these compositional techniques can be fully automated using AI algorithms. One of the most tedious postprocessing tasks often required for quantification of spatial or pixel information is image segmentation, which is typically performed on isotropic 3D MRI sequences. Segmentation is a complex task, and commonly used automation methods often still require substantial user input. However, recently developed segmentation techniques using deep learning convolutional neural networks and generative adversarial networks can segment knee articular cartilage and menisci in a fully automated fashion with accuracy comparable with that seen with segmentation performed by humans (– Fig. 12).^{23,44}

With these advances in postprocessing techniques and emerging acceleration techniques, the ability to incorporate quantitative MRI techniques into routine clinical protocols is now becoming feasible. As a consequence, the inclusion of 3D sequences as part of a routine knee MRI protocol is only likely to increase, given that these compositional techniques can directly use 3D acquisitions and are often paired with a morphological 3D sequence.

Conclusion

Three-dimensional sequences are being increasingly incorporated into knee MRI protocols due to the availability of new sequences such as 3D FSE, advanced metal artifact reduction techniques, and quantitative cartilage imaging with coincident advances in MRI acceleration techniques, such as parallel imaging, compressed sensing, and deep learning. Although 3D sequences are still primarily being used in addition to 2D sequences for morphological imaging, 3D sequences are increasingly replacing 2D sequences in certain applications, such as MR neurography and metal artifact reduction imaging. Furthermore, reductions in acquisition times of 3D compositional sequences, such as T1 ρ and T2 maps with compressed sensing and machine learning

acceleration techniques, in addition to fully automated segmentation algorithms, now make it feasible to incorporate these sequences clinically. As further advances and refinements in knee MRI acceleration, automation, and quantification techniques occur, 3D knee MRI will continue to become more accessible and valuable to clinical practices.

Conflict of Interest

None declared.

Acknowledgments

We would like to thank Megan Griffiths for help in the editing and preparation of this manuscript. We would also like to acknowledge several individuals working and collaborating with Dr. Xiaojuan Li and the Program of Advanced Musculoskeletal Imaging for their contributions in creating the figures in the “Emerging Techniques” section of this review: Jeehun Kim, Sibaji Gaj, Mingrui Yang, Kunio Nakamura, Leslie Ying, Chaoyi Zhang, and Hongyu Li.

References

- Shakoor D, Guerhazi A, Kijowski R, et al. Diagnostic performance of three-dimensional MRI for depicting cartilage defects in the knee: a meta-analysis. *Radiology* 2018;289(01):71–82
- Shakoor D, Kijowski R, Guerhazi A, et al. Diagnosis of knee meniscal injuries by using three-dimensional MRI: a systematic review and meta-analysis of diagnostic performance. *Radiology* 2019;290(02):435–445
- Altahawi F, Subhas N. 3D MRI in musculoskeletal imaging: current and future applications. *Curr Radiol Rep* 2018;6(08):27
- Kijowski R, Davis KW, Woods MA, et al. Knee joint: comprehensive assessment with 3D isotropic resolution fast spin-echo MR imaging—diagnostic performance compared with that of conventional MR imaging at 3.0 T. *Radiology* 2009;252(02):486–495
- Subhas N, Kao A, Freire M, Polster JM, Obuchowski NA, Winalski CS. MRI of the knee ligaments and menisci: comparison of isotropic-resolution 3D and conventional 2D fast spin-echo sequences at 3 T. *AJR Am J Roentgenol* 2011;197(02):442–450
- Jung JY, Yoon YC, Kwon JW, Ahn JH, Choe BK. Diagnosis of internal derangement of the knee at 3.0-T MR imaging: 3D isotropic intermediate-weighted versus 2D sequences. *Radiology* 2009;253(03):780–787

- 7 Ristow O, Steinbach L, Sabo G, et al. Isotropic 3D fast spin-echo imaging versus standard 2D imaging at 3.0 T of the knee—image quality and diagnostic performance. *Eur Radiol* 2009;19(05):1263–1272
- 8 Kijowski R, Blankenbaker DG, Woods M, Del Rio AM, De Smet AA, Reeder SB. Clinical usefulness of adding 3D cartilage imaging sequences to a routine knee MR protocol. *AJR Am J Roentgenol* 2011;196(01):159–167
- 9 Crema MD, Roemer FW, Marra MD, et al. Articular cartilage in the knee: current MR imaging techniques and applications in clinical practice and research. *Radiographics* 2011;31(01):37–61
- 10 Van Dyck P, Gielen JL, Vanhoenacker FM, et al. Diagnostic performance of 3D SPACE for comprehensive knee joint assessment at 3 T. *Insights Imaging* 2012;3(06):603–610
- 11 Talbot BS, Weinberg EP. MR imaging with metal-suppression sequences for evaluation of total joint arthroplasty. *Radiographics* 2016;36(01):209–225
- 12 Garwood ER, Recht MP, White LM. Advanced imaging techniques in the knee: benefits and limitations of new rapid acquisition strategies for routine knee MRI. *AJR Am J Roentgenol* 2017;209(03):552–560
- 13 Chhabra A, Madhuranthakam AJ, Andreisek G. Magnetic resonance neurography: current perspectives and literature review. *Eur Radiol* 2018;28(02):698–707
- 14 Madhuranthakam AJ, Lenkinski RE. Technical advancements in MR neurography. *Semin Musculoskelet Radiol* 2015;19(02):86–93
- 15 Ahlawat S, Carrino JA. Three-dimensional imaging of lower limb neuropathies. *Semin Musculoskelet Radiol* 2015;19(02):168–178
- 16 Gustas CN, Blankenbaker DG, Rio AM, Winalski CS, Kijowski R. Evaluation of the articular cartilage of the knee joint using an isotropic resolution 3D fast spin-echo sequence with conventional and radial reformatted images. *AJR Am J Roentgenol* 2015;205(02):371–379
- 17 Wang Y-XJ, Zhang Q, Li X, Chen W, Ahuja A, Yuan J. T1 ρ magnetic resonance: basic physics principles and applications in knee and intervertebral disc imaging. *Quant Imaging Med Surg* 2015;5(06):858–885
- 18 de Mello R, Ma Y, Ji Y, Du J, Chang EY. Quantitative MRI musculoskeletal techniques: an update. *AJR Am J Roentgenol* 2019;213(03):524–533
- 19 Guermazi A, Alizai H, Crema MD, Trattinig S, Regatte RR, Roemer FW. Compositional MRI techniques for evaluation of cartilage degeneration in osteoarthritis. *Osteoarthritis Cartilage* 2015;23(10):1639–1653
- 20 Roemer FW, Crema MD, Trattinig S, Guermazi A. Advances in imaging of osteoarthritis and cartilage. *Radiology* 2011;260(02):332–354
- 21 Recht MP, Zbontar J, Sodickson DK, et al. Using deep learning to accelerate knee MRI at 3 T: results of an interchangeability study. *AJR Am J Roentgenol* 2020;215(06):1421–1429
- 22 Subhas N, Li H, Yang M, et al. Diagnostic interchangeability of deep convolutional neural networks reconstructed knee MR images: preliminary experience. *Quant Imaging Med Surg* 2020;10(09):1748–1762
- 23 Gaj S, Yang M, Nakamura K, Li X. Automated cartilage and meniscus segmentation of knee MRI with conditional generative adversarial networks. *Magn Reson Med* 2020;84(01):437–449
- 24 Kalia V, Fritz B, Johnson R, Gilson WD, Raithel E, Fritz J. CAIPIRINHA accelerated SPACE enables 10-min isotropic 3D TSE MRI of the ankle for optimized visualization of curved and oblique ligaments and tendons. *Eur Radiol* 2017;27(09):3652–3661
- 25 Altahawi FF, Blount KJ, Morley NP, Raithel E, Omar IM. Comparing an accelerated 3D fast spin-echo sequence (CS-SPACE) for knee 3-T magnetic resonance imaging with traditional 3D fast spin-echo (SPACE) and routine 2D sequences. *Skeletal Radiol* 2017;46(01):7–15
- 26 Fritz J, Ahlawat S, Demehri S, et al. Compressed sensing SEMAC: 8-fold accelerated high resolution metal artifact reduction MRI of cobalt-chromium knee arthroplasty implants. *Invest Radiol* 2016;51(10):666–676
- 27 Fritz J, Raithel E, Thawait GK, Gilson W, Papp DF. Six-fold acceleration of high-spatial resolution 3D SPACE MRI of the knee through incoherent k-space undersampling and iterative reconstruction—first experience. *Invest Radiol* 2016;51(06):400–409
- 28 Kijowski R, Gold GE. Routine 3D magnetic resonance imaging of joints. *J Magn Reson Imaging* 2011;33(04):758–771
- 29 Naraghi A, White LM. Three-dimensional MRI of the musculoskeletal system. *AJR Am J Roentgenol* 2012;199(03):W283–293
- 30 Gold GE, Fuller SE, Hargreaves BA, Stevens KJ, Beaulieu CF. Driven equilibrium magnetic resonance imaging of articular cartilage: initial clinical experience. *J Magn Reson Imaging* 2005;21(04):476–481
- 31 Duc SR, Koch P, Schmid MR, Horger W, Hodler J, Pfirrmann CW. Diagnosis of articular cartilage abnormalities of the knee: prospective clinical evaluation of a 3D water-excitation true FISP sequence. *Radiology* 2007;243(02):475–482
- 32 Chen CA, Kijowski R, Shapiro LM, et al. Cartilage morphology at 3.0T: assessment of three-dimensional MR imaging techniques. *J Magn Reson* 2010;32(01):173–183
- 33 Busse RF, Hariharan H, Vu A, Brittain JH. Fast spin echo sequences with very long echo trains: design of variable refocusing flip angle schedules and generation of clinical T2 contrast. *Magn Reson Med* 2006;55(05):1030–1037
- 34 Gold GE, Busse RF, Beehler C, et al. Isotropic MRI of the knee with 3D fast spin-echo extended echo-train acquisition (XETA): initial experience. *AJR Am J Roentgenol* 2007;188(05):1287–1293
- 35 Pass B, Robinson P, Hodgson R, Grainger AJ. Can a single isotropic 3D fast spin echo sequence replace three-plane standard proton density fat-saturated knee MRI at 1.5 T? *Br J Radiol* 2015;88(1052):20150189
- 36 Del Grande F, Delcogliano M, Guglielmi R, et al. Fully automated 10-minute 3D CAIPIRINHA SPACE TSE MRI of the knee in adults: a multicenter, multireader, multifield-strength validation study. *Invest Radiol* 2018;53(11):689–697
- 37 Kijowski R, Davis KW, Blankenbaker DG, Woods MA, Del Rio AM, De Smet AA. Evaluation of the menisci of the knee joint using three-dimensional isotropic resolution fast spin-echo imaging: diagnostic performance in 250 patients with surgical correlation. *Skeletal Radiol* 2012;41(02):169–178
- 38 Zuo J, Li X, Banerjee S, Han E, Majumdar S. Parallel imaging of knee cartilage at 3 Tesla. *J Magn Reson Imaging* 2007;26(04):1001–1009
- 39 Frupp J, Crozier S, Warfield SK, Ourselin S. Automatic segmentation and quantitative analysis of the articular cartilages from magnetic resonance images of the knee. *IEEE Trans Med Imaging* 2010;29(01):55–64
- 40 Xia Y, Frupp J, Chandra SS, Walker D, Crozier S, Engstrom C. Automated 3D quantitative assessment and measurement of alpha angles from the femoral head-neck junction using MR imaging. *Phys Med Biol* 2015;60(19):7601–7616
- 41 Mars M, Chelli M, Tbini Z, Ladeb F, Gharbi S. MRI T2 mapping of knee articular cartilage using different acquisition sequences and calculation methods at 1.5 Tesla. *Med Princ Pract* 2018;27(05):443–450
- 42 Chhabra A, Lee PP, Bizzell C, Soldatos T. 3 Tesla MR neurography—technique, interpretation, and pitfalls. *Skeletal Radiol* 2011;40(10):1249–1260
- 43 Zare M, Faeghi F, Hosseini A, Ardekani MS, Heidari MH, Zarei E. Comparison between three-dimensional diffusion-weighted PSIF technique and routine imaging sequences in evaluation of peripheral nerves in healthy people. *Basic Clin Neurosci* 2018;9(01):65–71
- 44 Liu F, Zhou Z, Jang H, Samsonov A, Zhao G, Kijowski R. Deep convolutional neural network and 3D deformable approach for tissue segmentation in musculoskeletal magnetic resonance imaging. *Magn Reson Med* 2018;79(04):2379–2391
- 45 Ashinsky BG, Bouhrara M, Coletta CE, et al. Predicting early symptomatic osteoarthritis in the human knee using machine

- learning classification of magnetic resonance images from the osteoarthritis initiative. *J Orthop Res* 2017;35(10):2243–2250
- 46 Fritz J, Fritz B, Thawait GG, Meyer H, Gilson WD, Raithel E. Three-dimensional CAIPRINHA SPACE TSE for 5-minute high-resolution MRI of the knee. *Invest Radiol* 2016;51(10):609–617
- 47 Pandit P, Rivoire J, King K, Li X. Accelerated T1 ρ acquisition for knee cartilage quantification using compressed sensing and data-driven parallel imaging: a feasibility study. *Magn Reson Med* 2016;75(03):1256–1261